Quick Start Guide

Aco Apache Ultrasound System

Model: neo C62, neo L154, neo L187, neo P42, neo P3H

English

Product Overview


❶ System Status Indicator

❷ Power Key

❸


❹ Charging Status Indicator

❺

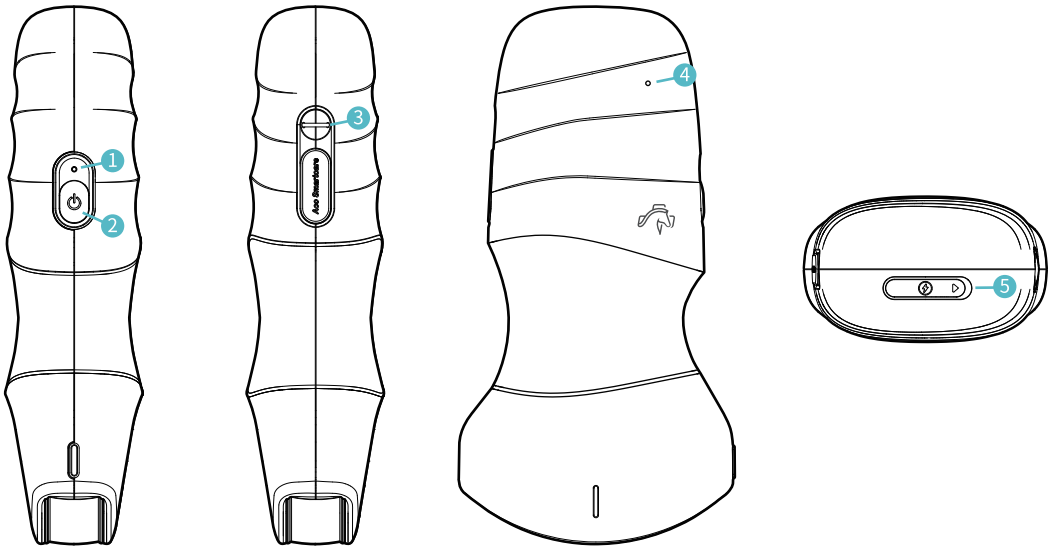

Indicator Description

Charging Status Indicator

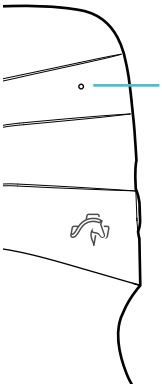





Blinking White:
when battery
capacity ≥ 20%



Blinking Yellow-Orange:
when battery
capacity < 20%



Steady White:
Charging completed




Fast blinking (2s):
battery low




Blinking yellow
orange and white:
battery abnormal

System Status Indicator

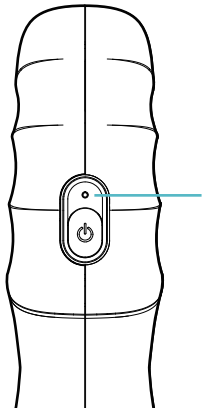





Fast blinking green:
ready for connection



Steady green: device
connects with mobile device



Slow blinking green:
booting




Steady yellow:
system abnormal

Hardware Setting

1 Step1: Charge device

Please charge 30 minutes before start using your device.


*Note: Please always use IEC60601 certified charger for device charging.

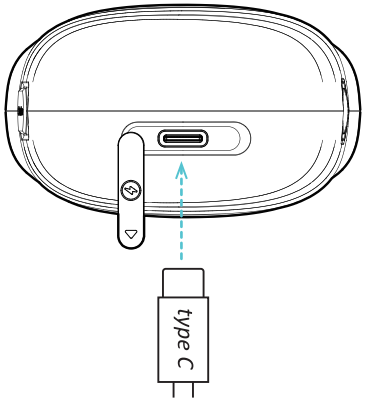

2 Step2: Power on/off

❶ Long press 1 second to power on your device.

❷ Long press for 3 seconds to power off your device.

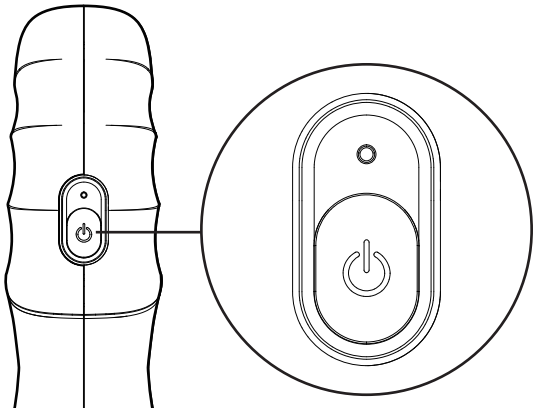

Install Apache App

1 Step1: Download App


Please scan the barcode as shown with your tablet or mobile devices.

GET IT ON Google Play


Download on the App Store

2 Step2: App configuration for Android

Please enable "Location" and "Overlay" setting while installing Apache App on Android.



Location: Please enable location by clicking "while using this app".




Overlay: Please enable overlay setting for "Apache App".

User Account Registration

1 Step1: Create New Account

Please click on "Create New Account" and complete your account registration.

*Note: Please ensure you have completed account registration before connecting to mobile device.

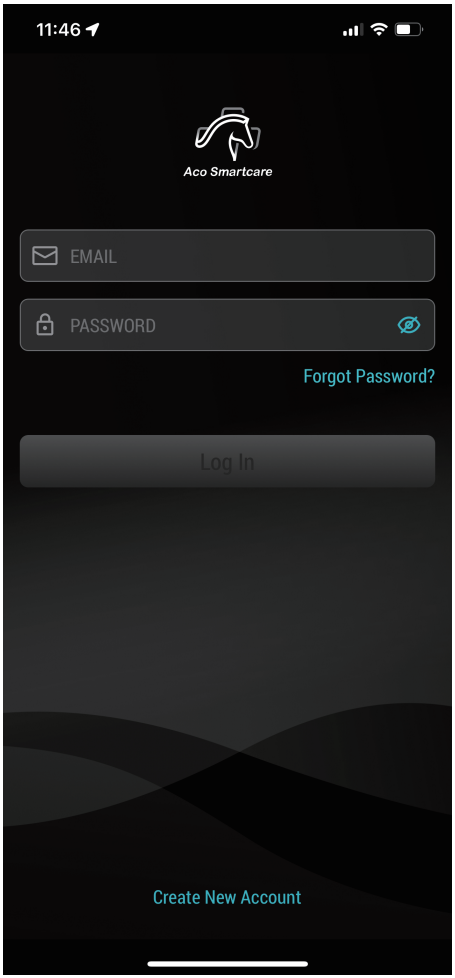

Probe Connection Instruction


1 Step1: Turn on Wi-Fi on your mobile/table

❶ Ensure Wi-Fi has been enabled on your device



2 Step2: Power on probe

Power on your probe and wait for 20 seconds to enter "ready for connect" status.

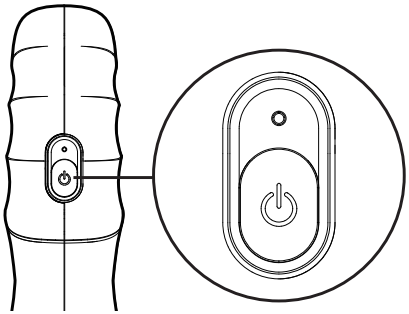

3 Step3:Way to connect the probe


Please use either one of the methods for device pairing.

❶ Scan the barcode printed on the probe rear cover.


❷ Select the probe on the probe list shown in the app.

*Note: Please always complete the "Add New Probe" procedure for the first use.

❶

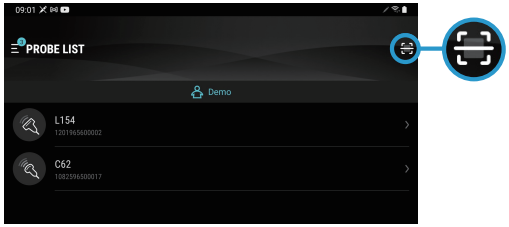

❷

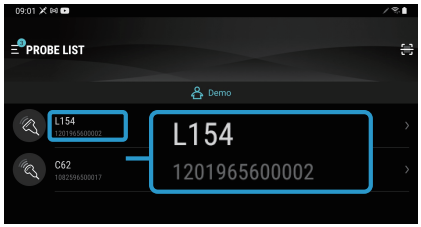

Aco Apache Ultrasound System is designed to be used by healthcare professionals in a professional healthcare environment.
MUST Read User Manual BEFORE use for full instructions, symbol glossary and safety information:
https://acohealthcare.com/downloads/

CE
1639

Manufacture:Aco Healthcare Co., Ltd
Email: service@acohealthcare.com

© 2020 Aco Smartcare
www.acohealthcare.com
All right reserved. No part of this publication may be reproduced or used in any form, or by any electrical or mechanical means, without permission in writing from Aco Smartcare. This includes electronic or mechanical means, such as photocopying, recording, or information storage and retrieval systems.

V2.0

FAQ