本產品是為受過培訓的專業人員所設計與被使用，
請詳閱本產品使用手冊之完整操作說明及安全資訊
www.acohealthcare.com/downloads

製造商: 奔騰智慧生醫股份有限公司
Email: service@acohealthcare.com

Aco Apache Vet Ultrasound System is designed to be used by professionals. Read User Manual for full instructions, symbol glossary and safety information: www.acohealthcare.com/download

Manufacture:Aco Healthcare Co., Ltd.
Email: service@acohealthcare.com

© 2020 Aco Smartcare
www.acohealthcare.com
All right reserved. No part of this publication may be reproduced or used in any form, or by any electrical or mechanical means, without permission in writing from Aco Smartcare. This includes electronic or mechanical means, such as photocopying, recording, or information storage and retrieval systems.

FAQ

Quick Start Guide

Aco Apache Vet Ultrasound System

Model: neo Vet series

Version 1.0

奔騰阿帕契獸用超音波系統

快速操作指南

產品外觀說明


Probe Connection Instruction

產品外觀說明


❶ **系統指示燈號**
System Status Indicator

❷ **電源鍵**
Power Key


❹ **充電指示燈**
Charing Status Indicator

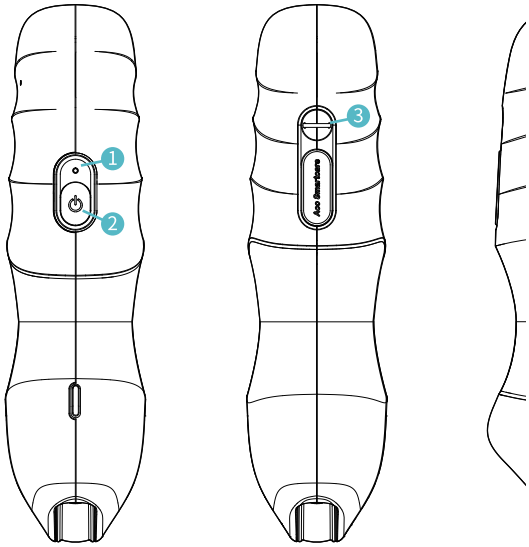

❶

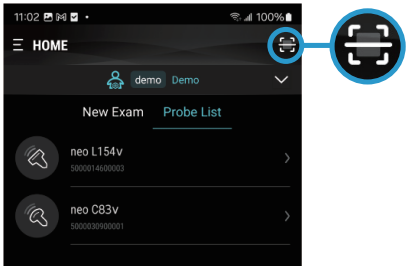

❷

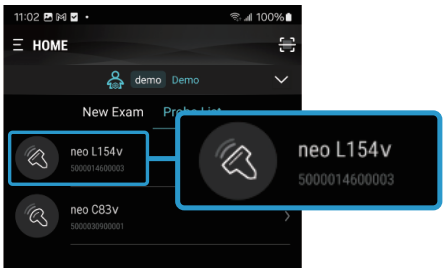

探頭連線操作

3 【步驟三】選擇連線方式

Step3: Way to connect the probe

選擇右方任一方式進行連線。

❶ 請用平板/手機掃描產品背後的Barcode來完成連線

Method 1: scan the barcode printed on the probe rear cover.

❷ 選擇您的探頭型號與序號進行配對

Method 2: select the probe on the probe list shown in the app.

***注意事項：若為首次註冊與連線之探頭，請先完成新增探頭之程序**


**Note: Please always complete the "Add New Probe" procedure for the first use*

❸ 吊繩孔

Lanyard hole

❺ 充電孔


Type-C Charing Port

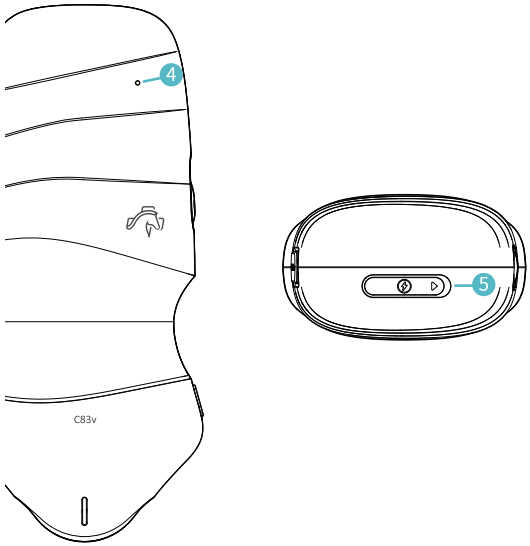

產品指示燈號說明

Probe Connection Instruction

充電指示燈

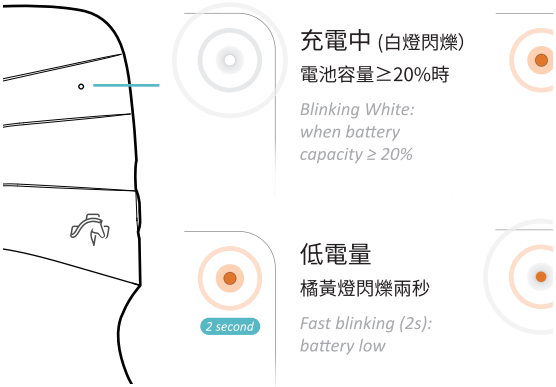

充電中 (白燈閃爍)

電池容量≥20%時

Blinking White: when battery capacity ≥ 20%


低電量

橘黃燈閃爍兩秒

Fast blinking (2s): battery low



系統指示燈

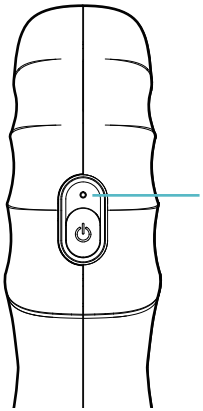




等待網路連線

綠燈快速閃爍


Fast blinking green: ready for connection



系統開機中

綠燈慢閃

Slow blinking green: booting

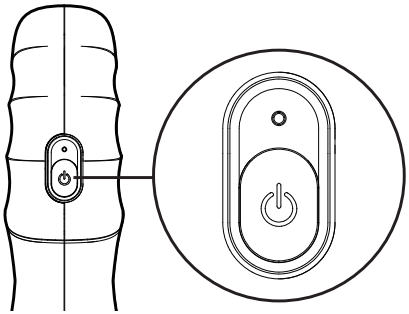

探頭連線操作

1 【步驟一】開啟Wi-Fi連線

Step1: Turn on Wi Fi on your mobile/table

❶ 確保手機/平板Wi-Fi已開啟

Ensure Wi-Fi has been enabled on your device

2 【步驟二】探頭開機

Step2: Power on probe

探頭開機，約20秒後，探頭進入等待連線模式。

Power on your probe and wait for 20 seconds to enter "ready for connect" status.

Indicator Description

Charging Status Indicator


充電中 (橘黃燈閃爍)
電池容量<20%時
Blinking Yellow-Orange: when battery capacity < 20%

充電完成 (白燈恆亮)
電池容量=100%
Steady White: Charging completed


電池異常
橘黃與白燈交互閃爍
Blinking yellow orange and white: battery abnormal

Note: 電量<20%時，請充電以保持電池健康度。

System Status Indicator



已完成網路連線
綠燈恆亮
Steady green: device connects with mobile device



系統異常
黃燈恆亮
Steady yellow: system abnormal

初始操作

User Account Registration

1 【步驟一】儀器充電

Step1: Charge device

打開電池保護蓋並且先充電30分鐘。

please charge 30 minutes before start using your device.

***注意事項：請選用通過IEC60601驗證的充電器來對您的產品進行充電。**

**Note: Please always use IEC60601 certified charger for device charging.*

2 【步驟二】探頭開機/關機操作


Step2: Power on/off

❶ 長按1秒開機

Long press 1 second to power on your device.

❷ 長按3秒關機


Long press for 3 seconds to power off your device.

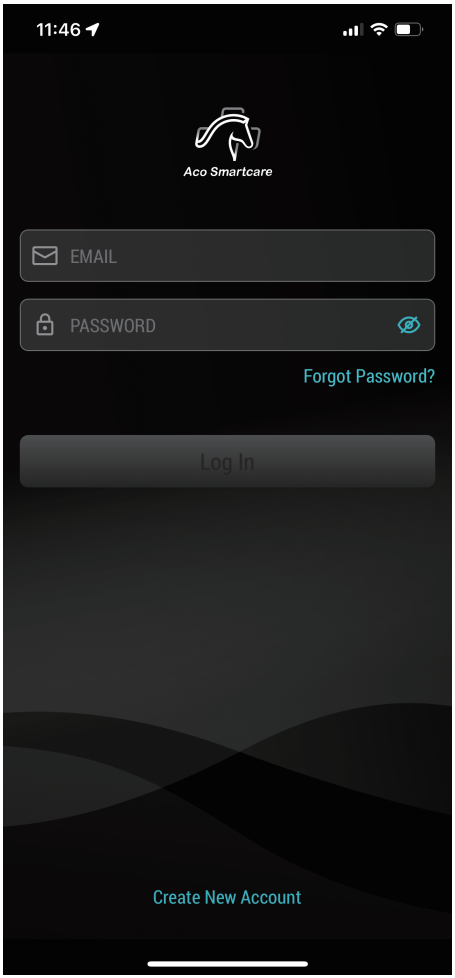

註冊帳號

1 【步驟一】建立新帳號

Sep1: Create New Account

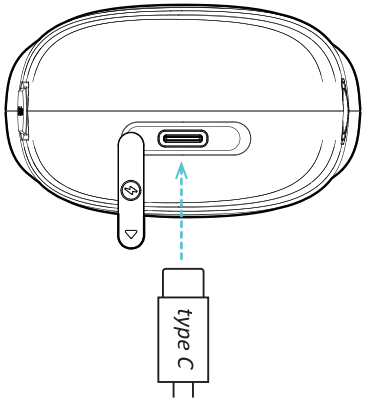


點選「建立新帳號」並且依照說明完成帳號註冊。

Please click on “Create New Account” and complete your account registration.

***注意事項：請確認註冊帳號已經完後後再進行探頭連線作業。**

**Note: Please ensure you have completed account registration before connecting to mobile device.*

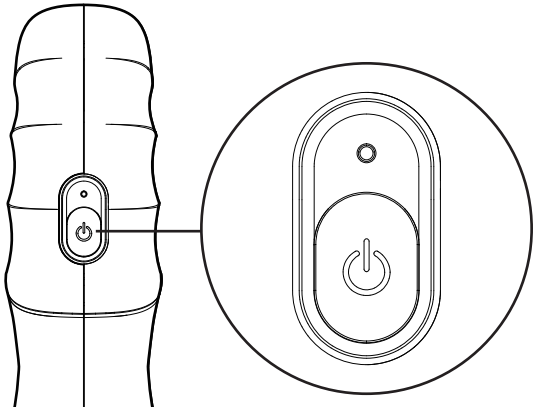

安裝APP

Install Apache App

1 【步驟一】下載App

Sep1: Download App

用手機/平板掃描右方2維碼進行App下載。


Please scan the barcode as shown with your tablet or mobile devices.

GET IT ON Google Play

Download on the App Store

2 【步驟二】Android App安裝設定

Step2: App configuration for Android






位置設定點選「使用此App時」。

Location: Please enable location by clicking "while using this app".

安裝Android App過程中，請依指示同意開啟「位置」及「畫面重疊」設定。

Please enable "Location" and "Overlay" setting while installing Apache App on Android.





圖層設定請點選「開啟設定」
並且把「Apache Vet」勾選打開。